Instruction Manual

8 Channel IEPE Conditioner

M208B

(from Version 002.006)



Manfred Weber

Metra Mess- und Frequenztechnik in Radebeul e.K.

Meissner Str. 58 - D-01445 Radebeul

Phone +49-351 836 2191 Fax +49-351 836 2940

Email: Info@MMF.de Internet: www.MMF.de

Manfred Weber Metra Mess- und Frequenztechnik in Radebeul e.K. Meissner Str. 58 D-01445 Radebeul Phone +49-351-836 2191 Fax +49-351-836 2940 Email Info@MMF.de Internet www.MMF.de

Notice: The current version of this document can be downloaded from http://www.mmf.de/product_literature.htm

Specifications subject to change without prior notice. © 2009 Manfred Weber Metra Mess- und Frequenztechnik in Radebeul e.K. No part of this document may be reproduced without the prior written consent of Metra.

Nov/ 22

Contents

1. Application	4
2. The Instrument at a Glance	4
2.1. Connectors and Controls	4
2.2. Menu Structure	5
3. What is IEPE?	5
4. Description of the Instrument	7
5. Power Supply	8
6. Inputs and IEPE Supply	9
7. Outputs	9
8. Grounding and Avoiding Ground Loops	10
9. Operation	10
9.1. Gain Selection	10
9.2. IEPE Indicators	10
9.3. Overload Indicators	10
9.4. Disabling Channel Monitoring	11
10. Filters and Integrators	11
10.1. Filters	11
10.2. Integrators	13
10.3. Replacing Filter Modules	15
10.4. Switching Off the High Pass Filters	16
10.5. Switching the IEPE Supply On or Off	17
10.6. Loading Default Settings	17
11. Calibration	17
12. Hardware and Software Version	18
13. Technical Data	19
Appendix: Warranty	

CE Declaration of Conformity

Thank you for using a vibration instrument from Metra!

1. Application


The 8 Channel IEPE Conditioner M208B was designed for piezoelectric accelerometers, force transducers, pressure transducers and measuring microphones with IEPE output. The instrument has the following functions:

- Constant current supply of up to eight sensors
- Gain ranges of 0, 20, 40 and 60 dB

2. The Instrument at a Glance

2.1. Connectors and Controls

Front Panel:

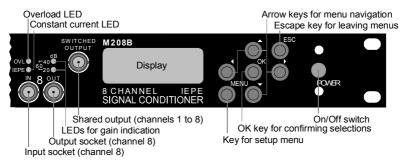


Rear Panel:



Figure 1: Front and rear panels

2.2. Menu Structure



3. What is IEPE?

The M208B is a signal conditioner for sensors with IEPE output. The abbreviation stands for Integrated Electronics Piezo Electric and is a common industrial standard for the output of piezoelectric sensors and microphones. Proprietary brand names, like ICP[®], Isotron[®], Deltatron[®], Piezotron[®] etc., are also used for the same purpose. An electronic circuit inside the sensor transforms the high-impedance signal of the sensing element into an output signal with low impedance, which can more easily be transmitted and processed.

A distinctive feature of IEPE is the transmission of supply current and measuring signal via one single wire, so an IEPE transducer is connected via a coaxial cable. 2 shows the principle circuit of an IEPE measuring chain. To supply the sensor elec-

tronics, constant current is used (not to be confused with 4-20 mA current loops). The constant current is fed into the signal cable by the signal conditioner. A coupling capacitor keeps the DC components away from the AC signal path.

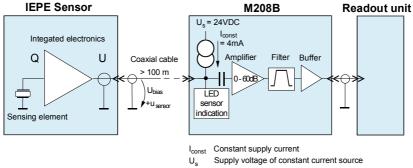


Figure 2: IEPE principle

When constant current is fed into the sensor, a positive DC voltage, called bias voltage, arises at the sensor terminals. Depending on model and manufacturer, the bias voltage can be in the range from 5 to 14 V. The bias voltage is modulated with the measuring signal u_{sensor} . The sensor output can never become negative. The minimum output voltage is approximately 1 V, the saturation voltage of the sensor output stage. The upper voltage limit is determined by the supply voltage of the constant current source, also called compliance voltage. The M208B uses 24 V. 3 shows the dynamic range of an IEPE transducer.

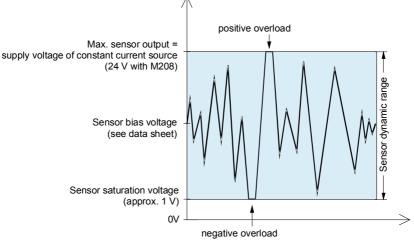


Figure 3: Dynamic range of IEPE sensors

The M208B features a circuit for sensor check. It can detect the following conditions, based on the sensor output voltage:

- No sensor: yellow LED off
- Sensor connected: yellow LED on
- Sensor shorted: yellow LED off

The constant current supply can be switched off for each channel (see section 10.5. on page 17). The sensor detection will then also be deactivated.

4. Description of the Instrument

4 shows the block diagram of the M208B. The instrument includes eight identical analog signal paths for amplification and filtering. A micro controller unit controls the analog part, provides digital interfaces, key control and display functions.

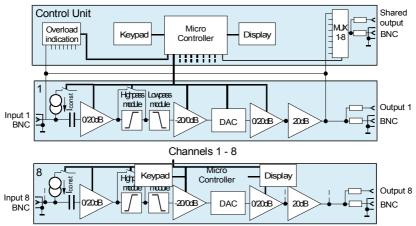


Figure 4: Block diagram

The sensor signals enter the M208B via BNC sockets on the front panel. The IEPE constant current sources may be switched off individually. The input is followed by an amplifier stage with selectable gains of 0 or 20 dB. High pass and low pass filters are designed as plug-in modules. The high pass can be switched off. There are also single and double integrator modules which may be plugged in instead of the filters. A selectable attenuator stage is followed by a digital-to-analog converter for gain calibration. Before the output there is another selectable amplifier stage and a buffer. Splitting the gain before and after the filters helps to avoid overload at frequencies in the filter stop band. The output is accessible on the front panel via BNC sockets. There is a shared output which can be switched to channels 1 to 8. The M208B is powered from a DC voltage source.

5. Power Supply

The M208B is powered by an external DC supply voltage between 10 and 28 V. This could be a supplied mains adapter or a car battery, for example. Current consumption is below 1.5 A. The supply voltage is connected by a circular power connector to DIN 45323. 5 shows the polarity of this socket.



Figure 5: Polarity of the supply socket

The M208B is protected against false polarization.

There is a fuse inside the instrument. For replacing the fuse, remove the four screws holding the cover plate and open the case. The location of the fuse holder is shown in 6. The fuse must be rated 2 A (slow).




Figure 6: Location of the fuse holder

- \Rightarrow Unplug the power supply before replacing the fuse!
- ⇒ Ground your hands before touching electronic components inside!
- \Rightarrow Use only fuses with the appropriate rating!

6. Inputs and IEPE Supply

The M208B has eight identical measuring channels. Sensors are connected via BNC sockets marked "IN" on the front panel. The input impedance is approximately 4 M Ω . The input overload limit is ± 10 V. The inputs can withstand voltages of up to ± 25 V.

For the operation with IEPE sensors constant current sources must be switched to the inputs (see 10.5 on page 17). By default the M208B is equipped with 4 mA constant current sources which is a practical value for most applications. For extremely long sensor cables and high frequencies to be measured, the instrument can also be equipped with 8 mA sensor supplies. The constant current source module can be replaced by the user. Open the cover plate after removing four screws (see 7).

- \Rightarrow Unplug the power supply before replacing the module!
- ⇒ Ground your hands before touching electronic components inside!

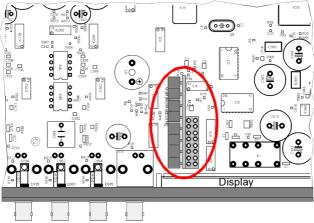


Figure 7: Location of the constant current source module

7. Outputs

The eight outputs are accessible via BNC sockets ("OUT") on the front panel. The outputs are short-circuit-proof. Their output impedance is 100Ω .

In addition to the channel outputs there is a shared output which can be connected to one of the channels. It is accessible via the BNC socket "SWITCHED OUTPUT" on the front.

The shared output is always connect to the channel which is underlined in the gain menu (see section 9.1). You may change the channel by pressing the $\triangleleft \triangleright$ keys.

8. Grounding and Avoiding Ground Loops

All inputs and outputs are referred to the same ground potential. Ground is also available at the socket ("GND") on the rear panel.

The negative supply Terminal (-) is also connected to ground.

To prevent ground loops it is recommended that additional connections are not made between the sensor cases via the test object. This can be avoided by using sensors with isolated base or isolating pads which are available as accessory parts.

9. Operation

9.1. Gain Selection

The instrument has four gain ranges of 0, 20, 40 and 60 dB (1, 10, 100 and 1000), which may be set for each channel individually.




Figure 8: Gain selection

After switching it on, the M208B displays the gain menu (8).

The selected gain ranges are shown over the respective channel numbers. The underlined value can be changed by the $\blacktriangle \lor$ keys. You may select between 0, 20, 40 and 60 dB. Change to another channel by $\blacklozenge \lor$. The active gains are also indicated by the LEDs over the output sockets:

0 dB:	LEDs off

20 dB: orange LED ("20")

- 40 dB: green LED ("40")
- 60 dB: orange and green LED

The gain settings remain stored when you disconnect the M208B from power.

Note: The underlined channel in the gain menu is also the channel connected to the shared output (see section 7).

9.2. IEPE Indicators

The yellow "IEPE" LED of an amplifier channel will light up when you connect a sensor to its input provided that the IEPE supply was switched on.

IEPE constant current indication is based on the measurement of the sensor bias voltage. If this voltage drops below 20 V the LED lights up.

9.3. Overload Indicators

Each channel has a red overload LED. The signal path is monitored for overload condition at the sensor and at the amplifier output to make sure that signal components which do not pass the filter but overload the input stage are properly indicated.

The threshold for the overload indicators is 10 V (peak). At this magnitude the signal is still undistorted.

Reduce the gain range when the overload LED starts flashing.

Please note that the dynamic range of most IEPE transducers is less than ± 10 V so that in the 0 dB range the signal may become clipped even if no overload is indicated.

9.4. Disabling Channel Monitoring

(from software version xxx.005)

For applications where highest resolution is demanded you can disable the periodic detection of sensor errors and overload which may cause glitches of approx. $0.5 \ \mu s$ and 50 mV every 5 s.

To do this press OK and ESC simultaneously. Confirm the two display messages by OK. Please note that IEPE sensor detection and overload indication will be disabled. The unit will return to normal operation after switching power off and on.

10. Filters and Integrators

10.1. Filters

High pass filters:		Low pass filters:	
3 dB frequency limit	Model	3 dB frequency limit	Model
3 Hz	FB3-3Hz	0.1 kHz	FB2-0.1kHz
5 Hz	FB3-5Hz	0.3 kHz	FB2-0.3kHz
10 Hz	FB3-10Hz	0.5 kHz	FB2-0.5kHz
30 Hz	FB3-30Hz	1 kHz	FB2-1kHz
50 Hz	FB3-50Hz	3 kHz	FB2-3kHz
100 Hz	FB3-100Hz	5 kHz	FB2-5kHz
300 Hz	FB3-300Hz	10 kHz	FB2-10kHz
500 Hz	FB3-500Hz	30 kHz	FB2-30kHz
1000 Hz	FB3-1000Hz	50 kHz	FB2-50kHz
		100 kHz	FB2-100kHz*

The M208B has replaceable high pass and low pass filter modules. The following frequencies are available:

* With the low pass FB2-100kHz at 60 dB gain and frequencies over 50 kHz the output peak voltage should not exceed \pm 3V to avoid distortion.

The high pass modules are second order Butterworth filters. The low pass modules are fourth order Butterworth filters.

The following diagrams show the frequency and phase response curves of the high pass and low pass filters.

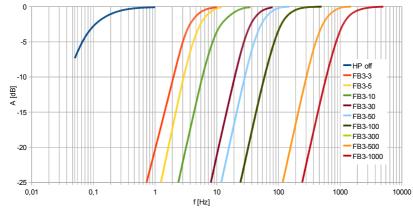


Figure 9: Frequency response of M208B with different high pass filters FB3-...

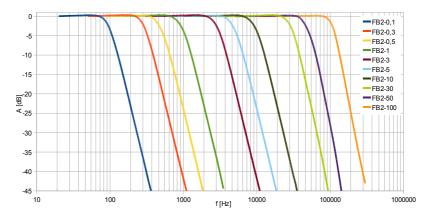


Figure 10: Frequency response of M208B with different low pass filters FB2-...

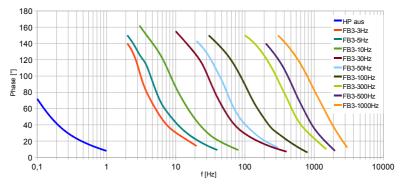


Figure 11: Phase response of M208B with different high pass filters FB3-...

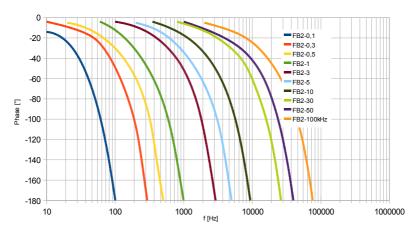


Figure 12: Phase response of M208B with different low pass filters FB2-...

10.2. Integrators

Integrators are useful to calculate vibration velocity or displacement from an acceleration input.

Single or double integrator modules can be plugged in instead of filters. Mixed filter operation is also allowed.

The single integrator FBV includes a second order 3 Hz high pass filter.

The double integrator FBD includes a second order 5 Hz high pass filter.

Figures 13 and 14 show the frequency response curves of the integrators.

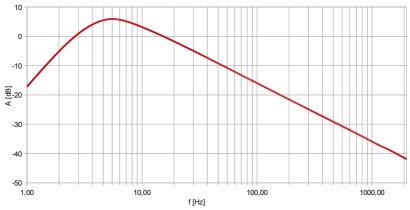


Figure 13: Frequency response of the M208B with the single integrator FBV

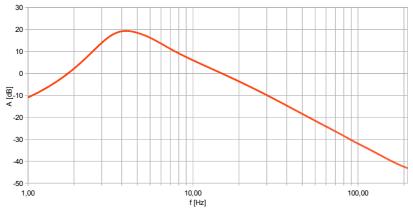


Figure 14: Frequency response of the M208B with the double integrator FBD

The following explanation is given to understand the relationship between the measured mechanical quantity and the integrated output of the M208B with an accelerometer:

The calculations show how the M208B output \mathbf{u}_{out} corresponds to the three vibration quantities. The selected gain range of the M208B is **G** (1, 10, 100 or 1000) and the accelerometer sensitivity (see transducer data sheet) is **B**_{ua}. Vibration acceleration a (without integration):

$$a = \frac{u_{out}}{G \cdot B_{ua}}$$

(a in m/s²; u_{out} in mV; B_{ua} in mV/ms⁻²)

Vibration velocity v (single integration):

$$v = \frac{u_{out}}{G \cdot B_{ua}} \cdot 10 s$$

(v in mm/s; u_{out} in mV; B_{ua} in mV/ms⁻²; s = seconds)

Vibration displacement d (double integration):

$$d = \frac{u_{out}}{G \cdot B_{ua}} \cdot 100 \, s^2$$

(d in μ m; u_{out} in mV; B_{ua} in mV/ms⁻²; s = seconds)

Example:

Vibration velocity is measured using an accelerometer with a sensitivity of $B_{qa} = 5 \text{ mV/ms}^2$. The M208B is operated in the range G = 100. Its output voltage is 300 mV_{ms}. What is the corresponding vibration velocity?

Solution:

$$v = \frac{300 \, mV}{100 \cdot 5 \, mV \, / ms^{-2}} \cdot 10 \, s = 6 \, mm \, / \, s_{eff}$$

When a direct connection between the output voltage of the M208B and the measured physical quantity should be desired (for example "1 mV corresponds to 1 mm/s"), you may may normalize the M208B output in the measuring equipment connected to its output or in the software.

The frequency range is limited to approximately 6 to 2000 Hz for single integration and 6 to 200 Hz for double integration. At the upper end of the frequency range only a poor signal-to-noise ratio can be achieved. This is the consequence of the freguency characteristic of electronic integrators.

It is not recommended to switch off the high pass function (see section 10.4) if integrator modules are used. The high pass filters inside the integrator modules have been designed in order to suppress low frequency noise which would appear at the amplifier output.

10.3. Replacing Filter Modules

For replacing filters or integrators, remove the four screws of the cover plate and open the case.

- ⇒ Unplug the power supply before replacing filters!
- ⇒ Ground your hands before touching electronic components inside!

15 shows the filter and integrator modules. Each channel has a high pass and a low pass module. Instead of the high pass and a low pass module an integrator module can be inserted. Pull out the modules carefully without bending their pins. When in-

serting the filter or integrator, make sure that the "Pin 1" mark ($\mathbf{\nabla}$) faces to the correct side.

For proper function of the M208B it is necessary that all filters or integrators are inserted.

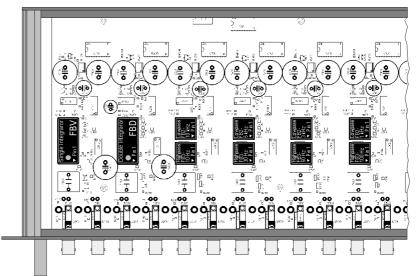


Figure 15: Location of the filter and integrator modules

10.4. Switching Off the High Pass Filters



Figure 16: Switching high pass filters on or off

- ⇒ Notice: When the high pass filter is switched off, low frequency noise from the sensor electronics and the constant current source may pass the signal path. It may appear as a fluctuating voltage at the amplifier output.
- ➡ It is not recommended to switch off the high pass function if integrator modules are used. The high pass filters inside the integrator modules have been de-

signed in order to suppress low frequency noise which would appear at the amplifier output.

10.5. Switching the IEPE Supply On or Off

IEPE transducers need a constant current supply for operation (compare section 3 on page 5). For measurements with other sensor types or for using the M208B as AC amplifier, it may be necessary to switch off the constant current sources. This can be done for each channel separately. Press the MENU key and open the menu "2/4: IEPE supply".



Figure 17: Switching the IEPE supply on or off

Use the keys $\blacktriangle \lor \checkmark \lor \lor$ to disable (\circ) or enable (\bullet) the constant current source of the respective channel. Confirm with OK or press ESC to quit without changes. When the IEPE supply is switched off, the M208B works as voltage amplifier with the gains 0/20/40/60 dB.

➡ It is recommended that the IEPE supply of unused channels be kept switched on in order to terminate the inputs. Otherwise electromagnetic interference via the unterminated inputs could induce noise in other channels.

10.6. Loading Default Settings

The M208B can be reset to its factory default settings in the menu "3/4: Load defaults". The following settings will be changed:

- Gain for all channels 0 dB
- All high pass filters switched off
- All IEPE constant current sources switched off

Calibration data is not changed.

11. Calibration

This section is intended only for users with sufficient experience in the field of the measurement of low AC signals and with precise measuring equipment of traceable accuracy.

We recommend a factory re-calibration at Metra after two years when the M208B was used under normal environmental conditions.

The M208B can be calibrated without opening the case. There are no adjustment points inside.

Click the MENU key to open the menu "4/4: Factory setup". This menu is password protected to avoid unwanted alteration. Enter the following password: "1410".

After opening the calibration menu the IEPE constant current sources and the high pass filters will be automatically switched off.

In some cases it may be desired to reset all calibration values to 0.0 % before calibration. This can be done by holding the MENU key while pushing the RESET key on the rear panel. Erasing the calibration values must be confirmed by OK.

Calibration is performed by feeding a sine-wave generator signal into all eight inputs simultaneously. No inputs must be left unterminated. Use "T" couplers and short BNC cables to interconnect the inputs. The generator frequency shall be 80 Hz and the RMS value 5.000, 50.00, 500.0 or 5000 mV, depending on the gain range to be calibrated. In addition to the generator, a calibrated RMS voltmeter should be connected to the inputs.

The amplifier output voltage of all channels is measured at the connector "SWITCHED OUTPUT" with a second calibrated RMS voltmeter. The signal quality at the outputs should also be monitored with an oscilloscope.

Select the channel to be calibrated ("Channel No.:", 1 to 8) and the gain range ("Gain range", 0/20/40/60 dB) by the $\blacktriangle \forall$ keys. Feed in the generator signal according to the display of the M208B, for example 50.00 mV in the gain range 40 dB.

The M208B will display the previously entered calibration value in percent, for example "-0.3%". Change this value by the $\blacktriangle \lor$ keys in steps of 0.1 % until the output voltage is exactly 5000 mV (RMS). Limits for calibration are ±2 %. Press OK to save your adjustment and to switch to the next channel or gain range.

12. Hardware and Software Version

The version number of your M208B is displayed for two seconds after switching on power.

The format of the version number is xxx.yyy with the hardware version xxx and the firmware version yyy. The line beneath shows the firmware upload date.



Figure 18: Version number

13. Technical Data

Inputs	8 voltage inputs; single-ended; $R_1 = 4 M\Omega$ AC coupled; IEPE compatible; BNC sockets $\pm 10 V$ without clipping at 0 dB gain $\pm 25 V$ peak input voltage
IEPE sensor supply	3.8 to 5.6 mA constant current; switchable compliance voltage > 22 V constant current indication by LED
Suitable sensors	IEPE compatible accelerometers, force transducers, pressure transducers and measuring microphones
Gains	0 / 20 / 40 / 60 dB
Gain accuracy	<0.3 % of nominal value at T=15 to 25 °C; U_a =1 to 5 V (RMS); f=80 Hz; high pass off; low pass 100 kHz
Noise (wide band) (0.1 Hz - 30 kHz)	0/20 dB: < 0,5 mV $_{_{RMS}}$; 40 dB: < 1 mV $_{_{RMS}}$; 60 dB: < 10 mV $_{_{RMS}}$
Noise densities	$\begin{array}{llllllllllllllllllllllllllllllllllll$
Cross-talk attenuation	> 80 dB
Frequency range	0.1 to 100 000 Hz (-3 dB); max. ± 3 V output at 60 dB and > 50 kHz
High pass filters	Plug-in modules: 3 / 5 / 10 / 30 / 50 / 100 / 300 / 500 / 1000 Hz frequency tolerance \pm 10%; 2nd order Butterworth filter
Low pass filters	Plug-in modules: $0.1/0.3/0.5/1/3/5/10/30/50/100$ kHz frequency tolerance $\pm 10\%$; 4 th order Butterworth filter
Integrators	Single integrator module FBV; double integrator module FBD
Outputs	8 buffered channel outputs; $\pm 10 \text{ V}$;100 Ω , BNC 1 buffered shared output; $\pm 10 \text{ V}$;100 Ω ; BNC output offset voltage: $< 3 \text{ mV}$
Overload indication	at sensor input and at at output by LEDs; threshold ± 10 V
Warm-up time	5 min
Power supply	10 to 28 V DC; < 1.5 A; DIN 45323 power connector
Operating temperature range	-10 to 50 °C
Dimensions	483 mm (19") x 44 mm (1 HU) x 124 mm
Weight	1.7 kg

Limited Warranty

Metra warrants for a period of 24 months

that its products will be free from defects in material or workmanship and shall conform to the specifications current at the time of shipment.

The warranty period starts with the date of invoice. The customer must provide the dated bill of sale as evidence. The warranty period ends after 24 months.

Repairs do not extend the warranty period.

This limited warranty covers only defects which arise as a result of normal use according to the instruction manual.

Metra's responsibility under this warranty does not apply to any improper or inadequate maintenance or modification and operation outside the product's specifications.

Shipment to Metra will be paid by the customer. The repaired or replaced product will be sent back at Metra's expense.

